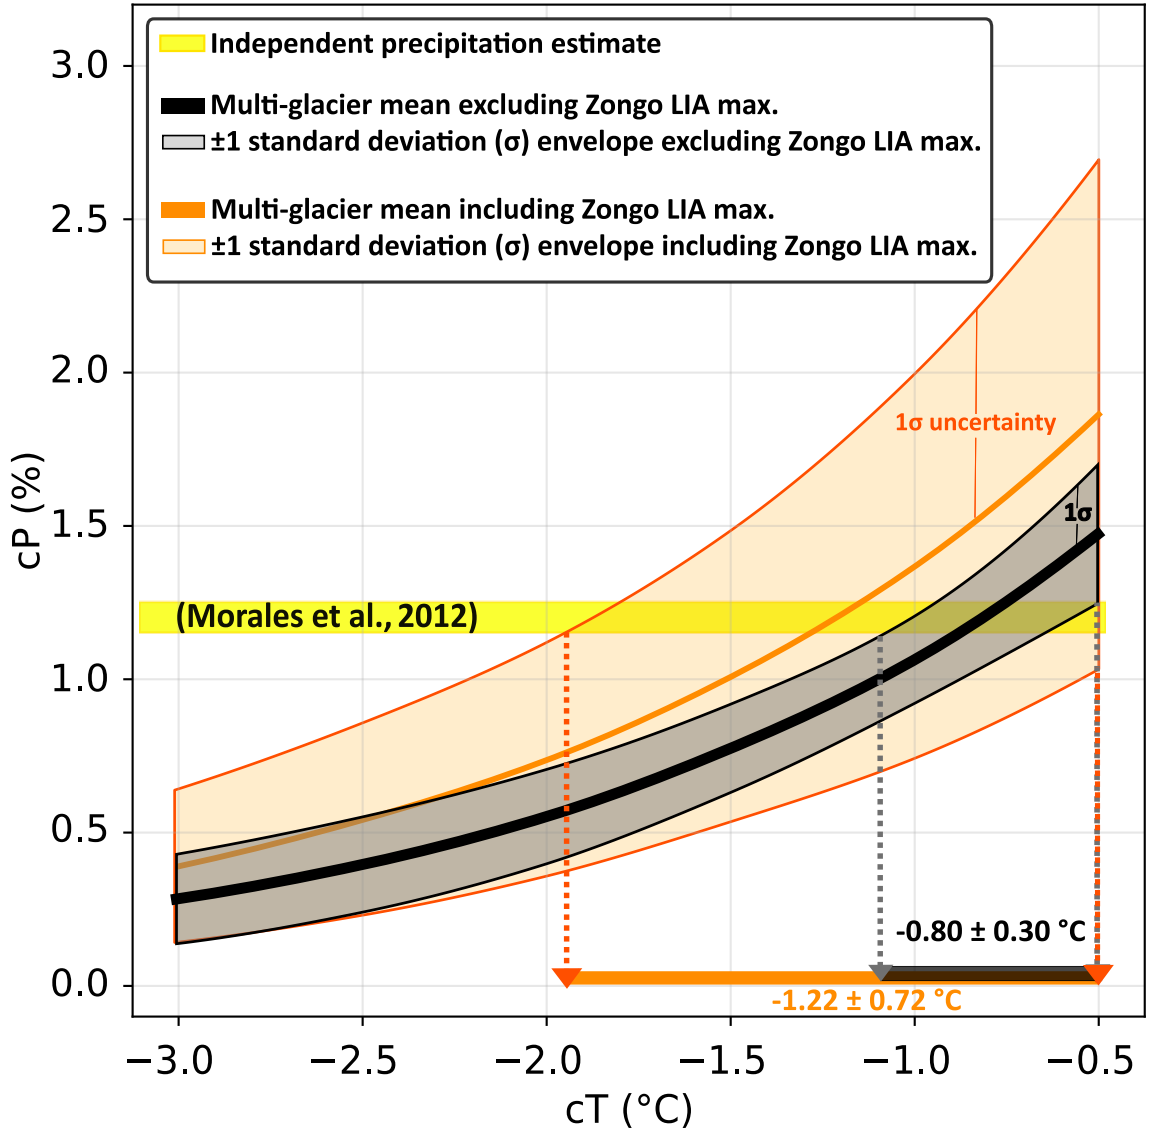

Independent precipitation estimate
Multi-glacier mean excluding Zongo LIA max.
±1 standard deviation (σ) envelope excluding Zongo LIA max.
Multi-glacier mean including Zongo LIA max.
±1 standard deviation (σ) envelope including Zongo LIA max.
1σ uncertainty
1σ
(Morales et al., 2012)
-0.80 ± 0.30 °C
-1.22 ± 0.72 °C
cP (%)
cT (°C)
3.0
2.5
2.0
1.5
1.0
0.5
0.0
−3.0
−2.5
−2.0
−1.5
−1.0
−0.5